

REVIN BRIELLE

Meet- en regeltechniek

Revision of instruments


TESTRAPPORT

Rapport nummer 3

	<u>Testinstrument</u>	<u>Instrument</u>
Instr. nummer	2276854	540173VW
Fabrikaat	Wika	Revin
Omschrijving	Digi Testmanometer	Manometer
Meetbereik	0-40 bar	0-25 bar
Klasse	0.1	1.0
Klant	TSH vakopleiding	
Getest door	B. Sewkaransing	

Meetpunten	Range Bar	Meetwaarde		Meetfout %	
		Stijgend	Dalend	Stijgend	Dalend
1	0,00	0,00	0,00	0,000	0,000
2	5,00	4,87	5,02	-0,520	0,080
3	10,00	9,78	9,87	-0,880	-0,520
4	15,00	14,76	14,83	-0,960	-0,680
5	20,00	19,77	19,85	-0,920	-0,600
6	25,00	24,79	24,79	-0,840	-0,840

Getest volgens DIN en 837-1: 1997

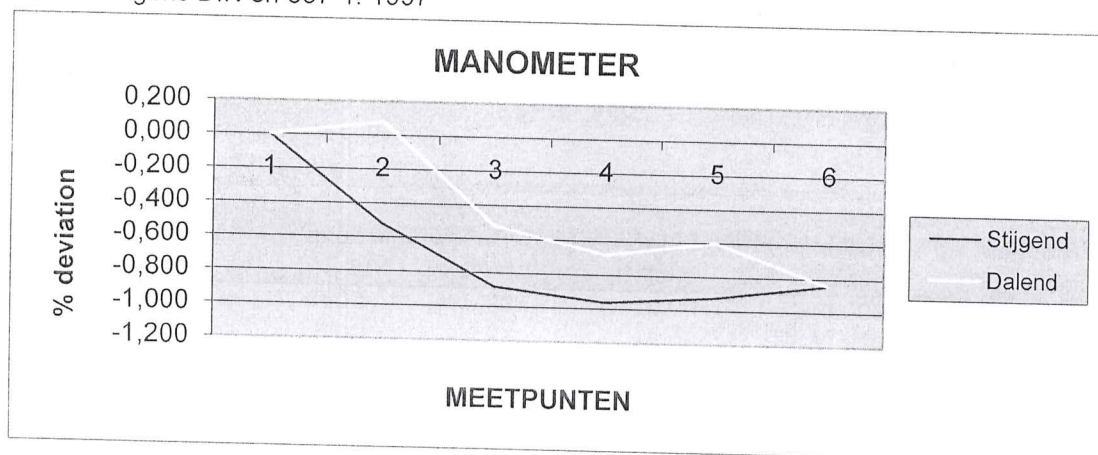

Datum 02-01-25
Ref. klant keuring
Ref. Revin 20240909

REVIN BRIELLE B.V.
't Woud 16
3332 LN Brielle
Tel: 0181-413094
e-mail: info@revinbrielle.com

Revin Brielle B.V. - Industrieterrein 't Woud 16, 3232 LN Brielle
Tel. (0181) 41 30 94 - E-mail info@revinbrielle.com - www.revinbrielle.com
Bank: Rabo. Rekeningnr. IBAN NR NL45RABO0344868680 - K.v.K. Rotterdam 24237422