

REVIN BRIELLE

Meet- en regeltechniek

Revision of instruments


TESTRAPPORT

Rapport nummer 3

	<u>Testinstrument</u>	<u>Instrument</u>
Instr.nummer	2276942	5405CB23
Fabrikaat	Wika	Revin
Omschrijving	Digi Testmanometer	Manometer
Meetbereik	0-2,5 bar	0-2,5 bar
Klasse	0.1	1.0
Klant	TSH Vakopleiding bv	
Getest door	B. Sewkaransing	

Meetpunten	Range Bar	Meetwaarde		Meetfout %	
		Stijgend	Dalend	Stijgend	Dalend
1	0,000	0,000	0,000	0,000	0,000
2	0,500	0,488	0,500	-0,480	0,000
3	1,000	0,982	0,995	-0,720	-0,200
4	1,500	1,481	1,492	-0,760	-0,320
5	2,000	1,977	1,990	-0,920	-0,400
6	2,500	2,476	2,476	-0,960	-0,960

Getest volgens DIN en 837-1: 1997

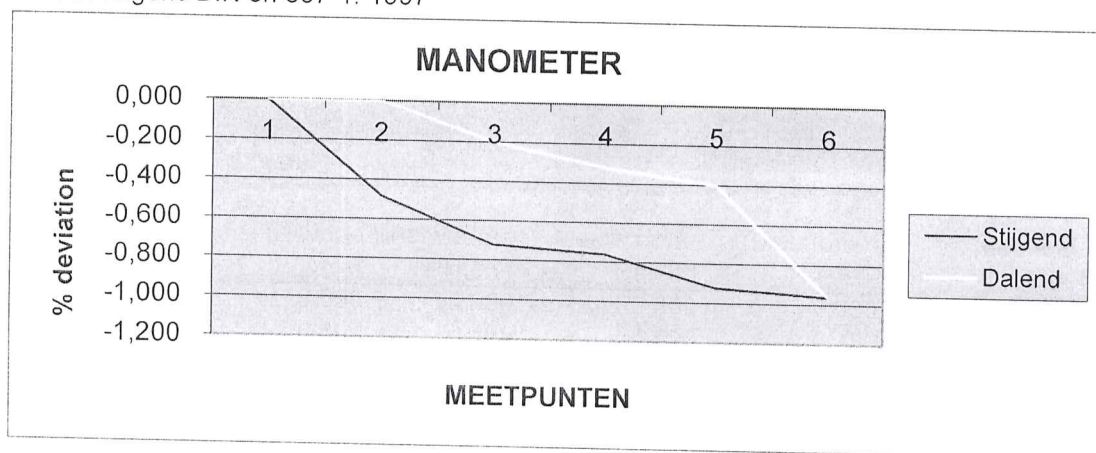

Datum 02-01-25
Ref. klant keuring
Ref. Revin 20240909

REVIN BRIELLE B.V.
't Woud 16
3232 LN Brielle
Tel: 0181-413094
e-mail: info@revinbrielle.com

Revin Brielle B.V. - Industrieterrein 't Woud 16, 3232 LN Brielle
Tel. (0181) 41 30 94 - E-mail info@revinbrielle.com - www.revinbrielle.com
Bank: Rabo. Rekeningnr. IBAN NR NL45RABO0344868680 - K.v.K. Rotterdam 24237422