


## TESTRAPPORT

Rapport nummer 3

	<u>Testinstrument</u>	<u>Instrument</u>
Instr.nummer	2276942	5405CB26
Fabrikaat	Wika	Revin
Omschrijving	Digi Testmanometer	Manometer
Meetbereik	0-2,5 bar	0-2,5 bar
Klasse	0.1	1.0
Klant	TSH Vakopleiding bv	
Getest door	B. Sewkaransing	

Meetpunten	Range Bar	Meetwaarde		Meetfout %	
		Stijgend	Dalend	Stijgend	Dalend
1	0,000	0,000	0,000	0,000	0,000
2	0,500	0,504	0,520	0,160	0,800
3	1,000	0,998	1,009	-0,080	0,360
4	1,500	1,485	1,491	-0,600	-0,360
5	2,000	1,983	1,993	-0,680	-0,280
6	2,500	2,488	2,488	-0,480	-0,480

Getest volgens DIN en 837-1: 1997

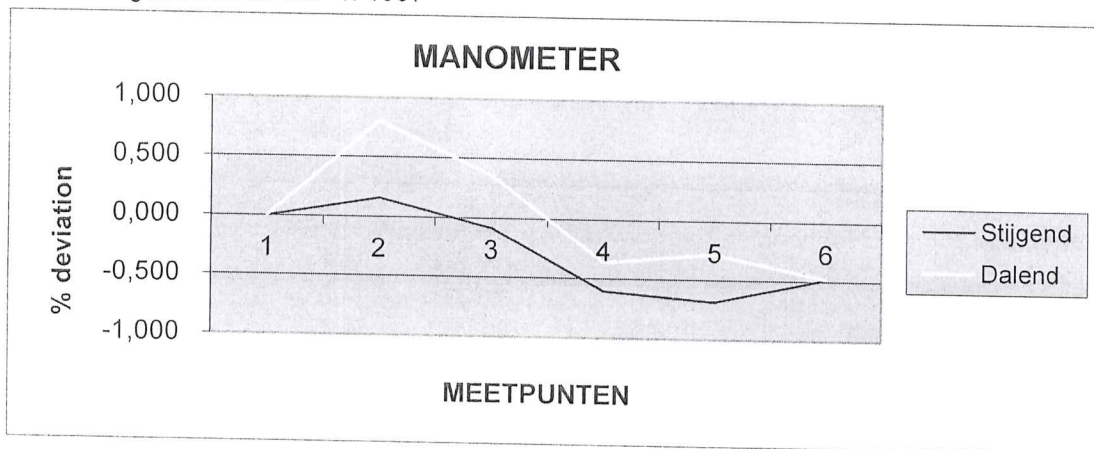

Datum 02-01-25  
Ref. klant keuring  
Ref. Revin 20240909

REVIN BRIELLE B.V.  
't Woud 16  
3232 LN Brielle  
Tel. 0181-413094  
e-mail: info@revinbrielle.com

Revin Brielle B.V. - Industrieterrein 't Woud 16, 3232 LN Brielle  
Tel. (0181) 41 30 94 - E-mail info@revinbrielle.com - www.revinbrielle.com  
Bank: Rabo. Rekeningnr. IBAN NR NL45RABO0344868680 - K.v.K. Rotterdam 24237422